


Software Version : 6.3.1.0504
Sample Name : SEMAX 10 mg SYNTHAGEN
Instrument Name : DIONEX
Rack/Vial : 0/0
Sample Amount : 1,000000
Cycle : 1

Date : 2023-03-18 18:55:27
Data Acquisition Time : 2023-03-03 12:43:30
Channel : B
Operator : manager
Dilution Factor : 1,000000

Result File :

Sequence File : C:\PenExe\TcWS\Ver6.3.1\Examples\IC-106-S\ROK 2023\MARZEC\02.03-peptydy\02.03.seq

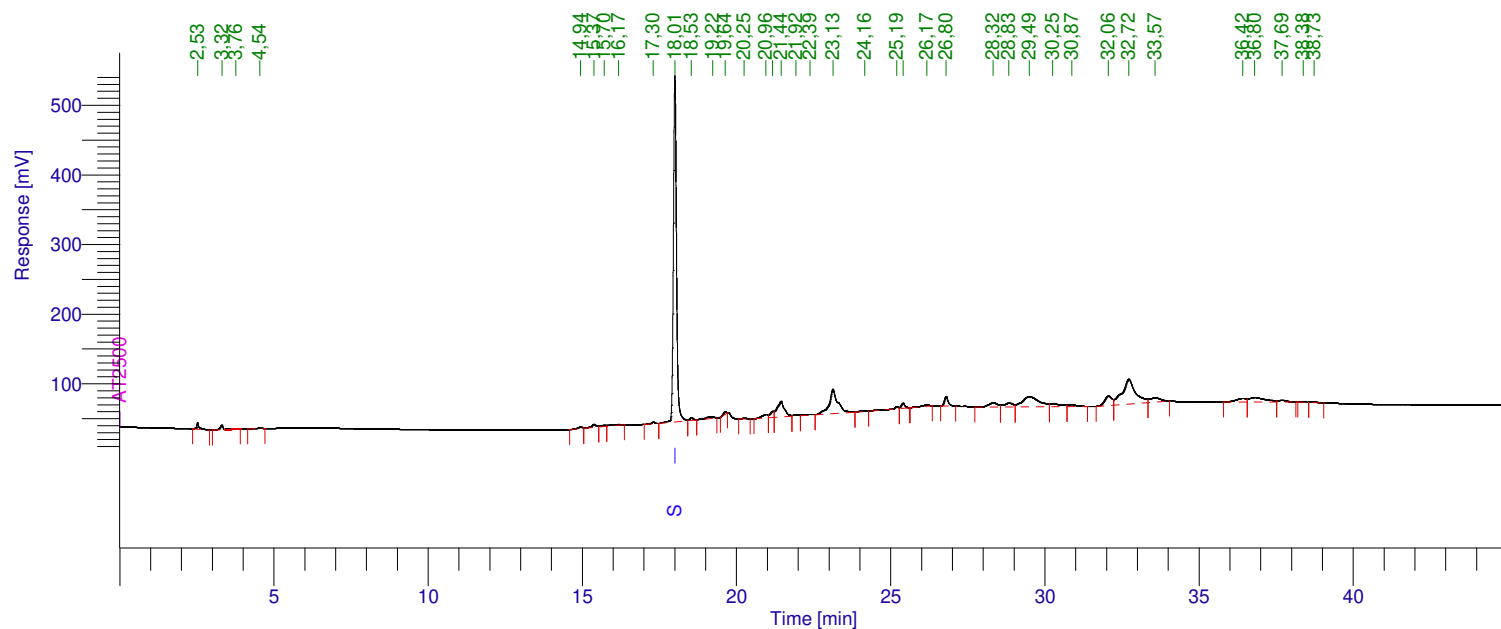

REPORT

Peak #	Component Name	Time [min]	Amount [mg/fiolka]
10	SEMAX	18,005	11,35

Eko-Analiza M.Turek, M.Wysocki sp.j.
ul. Harnasiow 9; 43-300 Bielsko-Biala
eko_analiza@onet.pl